
Tracing an anesthesia interface to the correct covers

QUESTION

Identify the device and Figure C interface, including its purpose. Trace the original and updated safety notices to the maintenance manual and guard-kit part numbers, including both covers. Can the older 1407-3333-000 port plug substitute? Name that part and its supported equipment.

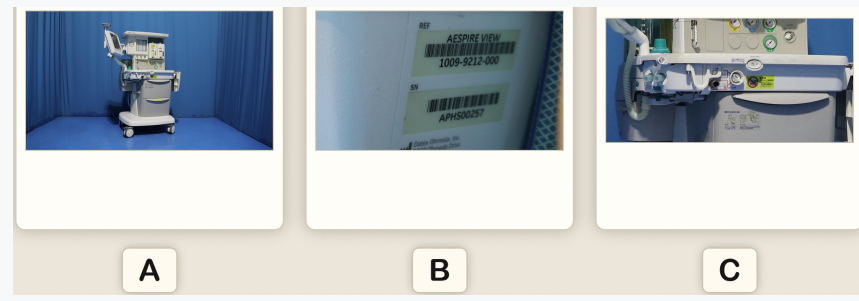

Input image

CONDENSED TRAJECTORY

[Goal]
Identify the pictured anesthesia system and Figure C interface, trace its safety notice and replacement covers, and check whether an older port plug can substitute.

[Observation]
The input image bears "AESPIRE VIEW".

[Tool Calls]
web_search(query="Aespire View field safety notice ACGO guard kit 1407-3333-000 port plug")
open_page(url="medicinesauthority.gov.mt/file.aspx?f=6955")

[Result]
Notice 34136 covers the Auxiliary Common Gas Outlet (ACGO) and selector switch. When selected, ACGO supplies fresh gas to auxiliary manual breathing systems; the remedy uses port and switch covers.

[Decision]
The first research report has not found the updated manufacturer reference or maintenance manual number. Continue searching.

[Tool Calls]
web_search(query="GE HealthCare Ref. # 34136 ACGO covers")
open_page(url="assets.hpra.ie/.../anaesthesia-system_ge-healthcare_advise-regarding-device-modification.pdf")

[Result]
Update 34136-TRM lists Aespire View manual M1170027.

[Tool Call] open_page(url="services.gehealthcare.com/.../1407-3333-000")

[Result]
This is a Breathing Circuit Gas (BCG) Circuit Port plug for the Aespire 7100 mounting structure.

[Tool Calls]
open_page(url="channelpartners.gehealthcare.com/.../2084453-001")
open_page(url="shop.gehealthcare.ca/.../2084453-001")

[Result]
Kit 2084453-001 corresponds to port cover 2075279-001 and switch cover 2075285-001.

[Final Answer]
Aespire View; ACGO port and switch. Notices: 34136 → 34136-TRM. Manual: M1170027. Required kit: 2084453-001, with the two identified covers. No: 1407-3333-000 is the older BCG port plug, not this cover remedy.